


Guideline for Management of COPD 2016-2018



SYMPTOMS

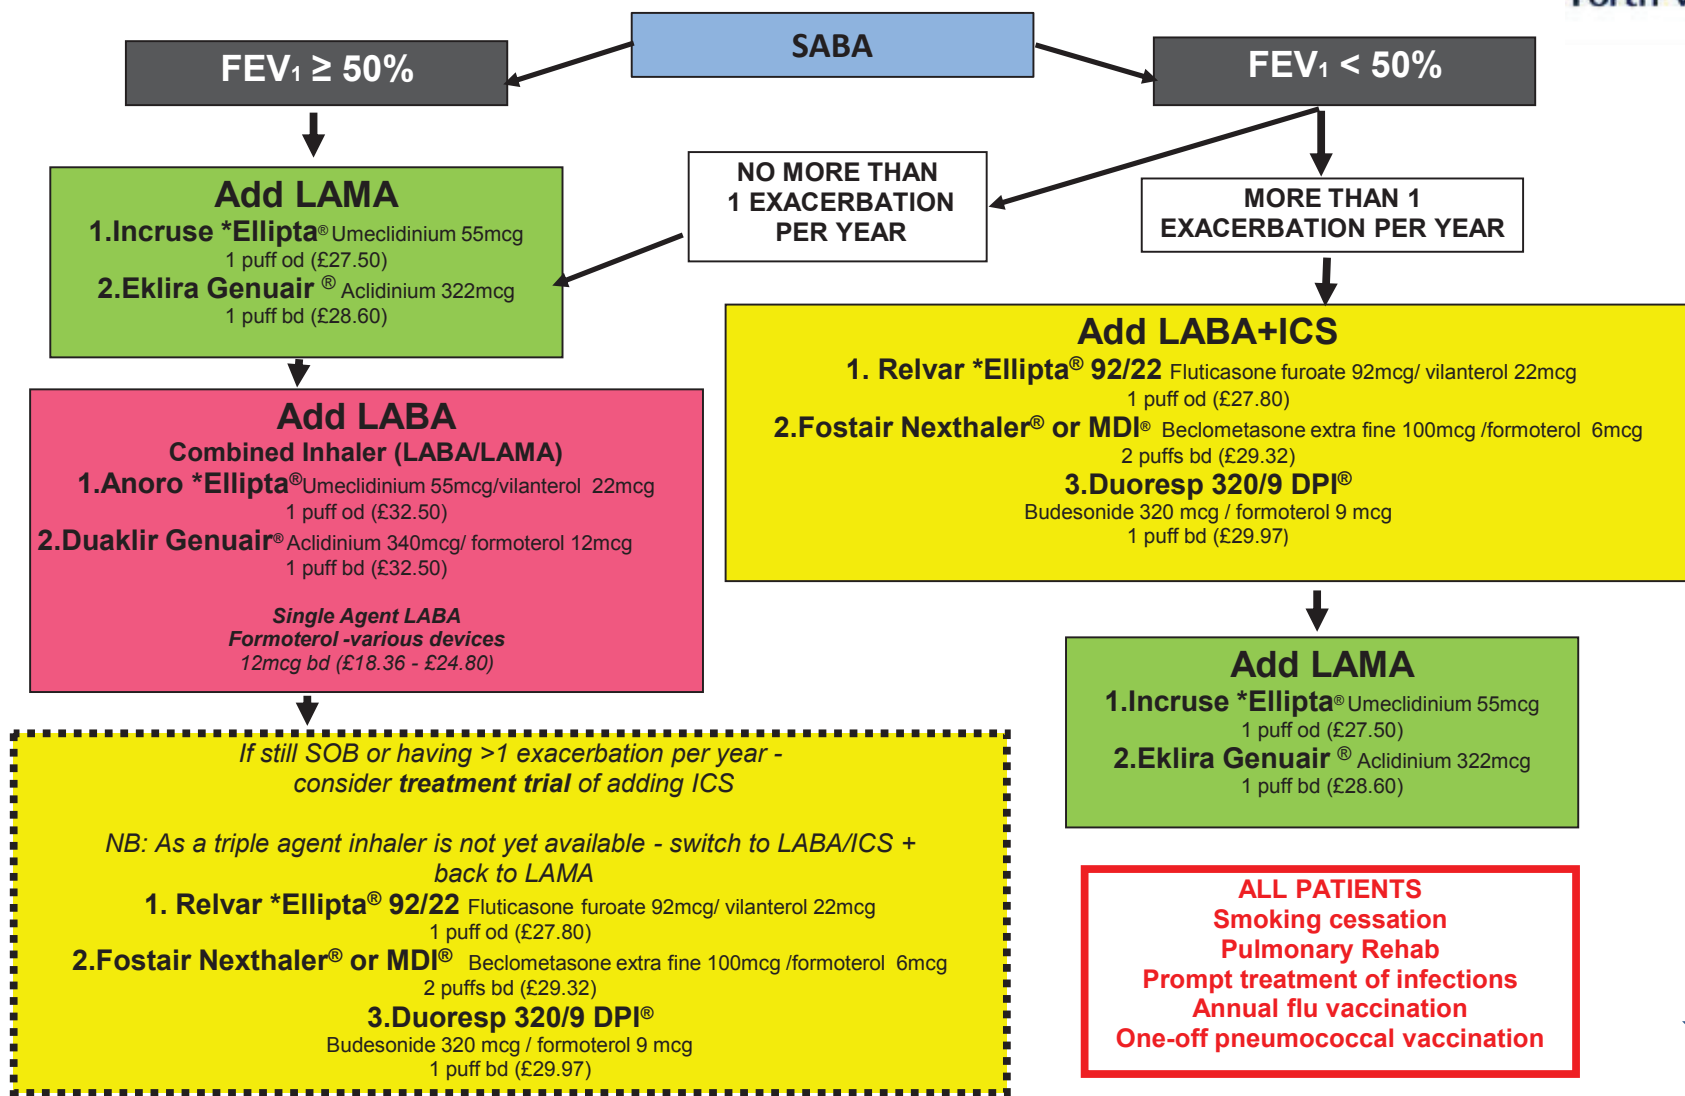

***NB - ELLIPTA® Devices only have a 6 week expiry once opened - advise patients to open and use ONE inhaler at a time and mark expiry when opening**
Fostair MDI requires refrigeration prior to dispensing and has a reduced expiry date of

Costs based on 30 days treatment at doses shown
 Reference: DM+D Accessed May 2015
 Developed by Clare Colligan
 Approved Airways MCN October 2015, PCPG Feb 2016